

NobelZygoma™ 45°

Instructions for use



Important: Please read.

Disclaimer of liability:

This product is part of an overall concept and may only be used in conjunction with the associated original products according to the instructions and recommendation of Nobel Biocare. Non-recommended use of products made by third parties in conjunction with Nobel Biocare products will void any warranty or other obligation, express or implied, of Nobel Biocare. The user of Nobel Biocare products has the duty to determine whether or not any product is suitable for the particular patient and circumstances. Nobel Biocare disclaims any liability, express or implied, and shall have no responsibility for any direct, indirect, punitive or other damages, arising out of or in connection with any errors in professional judgment or practice in the use of Nobel Biocare products. The user is also obliged to study the latest developments in regard to this Nobel Biocare product and its applications regularly. In cases of doubt, the user has to contact Nobel Biocare. Since the utilization of this product is under the control of the user, it is his/her responsibility. Nobel Biocare does not assume any liability whatsoever for damage arising thereof. Please note that some products detailed in this Instruction for Use may not be regulatory cleared, released or licensed for sale in all markets.

Description:

Implant:

NobelZygoma™ 45° implants are made from biocompatible commercially pure grade 4 titanium with TiUnite® surface. It is a parallel walled implant with a 45° abutment head. The implant has TiUnite® up to the level of the platform. The "Brånemark System® Zygoma TiUnite™" restorative assortment is to be used in combination with this implant due to the need for a shorter restorative screw.

The implant comes with a co-packed Cover Screw made of Titanium alloy Ti-6Al-4V.

Tooling:

Nobel Biocare Twist Drills and Pilot Drills are made of stainless steel with a DLC (Diamond Like Carbon) coating. Round Burs are made of stainless steel with no DLC (Diamond Like Carbon) coating. They should be used in conjunction with NobelZygoma™ 45° implants and are for single use only.

Zygoma Drill Guard, Zygoma Drill Guard Short, Zygoma Depth Indicator Straight and Zygoma Depth Indicator Angled are made of stainless steel. Zygoma Handle is made of aluminium alloy and stainless steel. They should be used in conjunction with NobelZygoma™ 45° implants and are intended for reuse.

Intended use:

NobelZygoma™ 45° implants are endosseous implants and are integrated in the zygomatic bone (osseointegration). They are intended to be used for anchoring or supporting tooth replacements to restore chewing function.

Indications:

NobelZygoma™ 45° implants are endosseous dental implants intended to be surgically placed in the bone of the upper jaw arches to provide support for prosthetic devices, such as artificial teeth, in order to restore patient esthetics and chewing function. These implants may be put into immediate function provided that stability requirements detailed in the directions for use are satisfied.

Contraindications:

NobelZygoma™ 45° implant is contraindicated for patients:

- who are medically unfit for an oral surgical procedure.
- with inadequate bone volume for conventional implants and zygoma implant(s).
- in whom adequate sizes, numbers or desirable position of implants are not reachable to achieve safe support of functional or eventually parafunctional loads.
- who are allergic or hypersensitive to commercially pure titanium grade 4 and grade 1, titanium alloy Ti-6Al-4V (titanium, aluminum, vanadium), stainless steel or DLC (Diamond Like Carbon) coating.
- who are to be restored with single unit constructions.

Warnings:

Failure to recognize actual lengths and direction of drills relative to radiographic measurements and surrounding anatomical structures can result in permanent injury to nerves or other surrounding vital structures.

Besides the mandatory precautions for any surgery such as asepsis, during drilling in the zygomatic bone, one must avoid damage to the nerves and vessels by referring to anatomical knowledge and preoperative radiographs.

In general the most notable risks associated with the Zygoma implants are sinusitis and fistula formations.

Cautions:

General:

One hundred percent implant success cannot be guaranteed. Especially, non-observance of the indicated limitations of use and working steps may result in failure.

Treatment by means of implants may lead to loss of bone, biologic or mechanical failures including fatigue fracture of implants.

Close cooperation between surgeon, restorative dentist and dental laboratory technician is essential for a successful implant treatment.

It is strongly recommended that NobelZygoma™ 45° implants are used only with Nobel Biocare surgical instruments and prosthetic components, as combining components that are not dimensioned for correct mating can lead to mechanical and/or instrumental failure, damage to tissue or unsatisfactory esthetic results.

It is strongly recommended that clinicians, new as well as experienced implant users, always go through special training before undertaking a new treatment method. Nobel Biocare offers a wide range of courses for various levels of knowledge and experience. For more information please visit www.nobelbiocare.com.

Working the first time with a colleague, experienced with the new device/treatment method, avoids eventual complications. Nobel Biocare has a global network of mentors available for this purpose.

Before surgery:

Careful clinical and radiological examination of the patient has to be performed prior to surgery to determine the psychological and physical status of the patient. It is highly recommended to perform a medical CT scan or a CBCT (cone beam CT) analysis prior to the final treatment decision. The patient must have clinically symptom-free sinuses, no pathology in associated bone and soft tissue and completed all necessary dental treatment.

Special attention has to be given to patients who have local or systemic factors that could interfere with the healing process of either bone or soft tissue or the osseointegration process (e.g., cigarette smoking, poor oral hygiene, uncontrolled diabetes, oro-facial radiotherapy, steroid therapy, infections in the neighboring bone). Special caution is advised in patients who receive bisphosphonate therapy.

In general, implant placement and prosthetic design must accommodate individual patient conditions. In case of bruxism or unfavorable jaw relationships reappraisal of the treatment option may be considered.

With respect to pediatric patients, routine treatment is not recommended until the end of the jaw bone growth phase has been properly documented.

Pre-operative hard tissue or soft tissue deficits may yield a compromised esthetic result or unfavorable implant angulation.

All instruments and tooling used during procedure must be maintained in good condition and care must be taken that instrumentation does not damage implants or other components.

Zygoma implants treatments could be performed under local anesthesia, IV-sedation or general anesthesia.

At surgery:

Care and maintenance of instruments are crucial for a successful treatment. Sterilized instruments not only safeguard your patients and staff against infection but are also essential for the outcome of the total treatment.

Because of the small size of components, care must be taken that they are not swallowed or aspirated by the patient.

NobelZygoma™ 45° implants may be tilted up to 45° relative to the occlusal plane. When used with angulations between 30° and 45°, the following applies: The tilted implant must be splinted; a minimum of 4 implants must be used when supporting a fixed prosthesis in a fully edentulous arch.

After the implant installation, the surgeon's evaluation of bone quality and primary stability will determine when implants may be loaded. Lack of adequate quantity and/or quality of remaining bone, infection and generalized diseases may be potential causes for failure of osseointegration both immediately after surgery, or after osseointegration is initially achieved.

Bending moments: Forces that cause bending moments are known to be the most unfavorable, as they can potentially jeopardize the long-term stability of an implant-supported restoration. In order to decrease bending moments, the distribution of forces should be optimized by cross-arch stabilization, minimizing distal cantilevers, having a balanced occlusion as well as decreased cuspal inclination of the prosthetic teeth.

After surgery:

To secure the long term treatment outcome it is advised to provide comprehensive regular patient follow-up after implant treatment and to inform about appropriate oral hygiene.

Surgical procedure:

1. To begin exposure of the lateral maxillary wall, a full thickness mucoperiosteal flap is reflected following a crestal incision with bilateral distal vertical releasing incisions over the tuberosity areas.

Warning: It is imperative to be aware of vital structures including nerves, veins and arteries during the surgical exposure of the lateral maxillary wall. Injuries to vital anatomic structures can lead to complications including injury to the eye as well as extensive bleeding and nerve-related dysfunction.


Image (A) highlights the following landmarks which may be used in keeping oriented during the anatomic dissection:

- a. Posterior wall of the maxillary sinus
- b. Zygomatic-maxillary buttress
- c. Infra-orbital foramen
- d. Fronto-zygomatic notch

Caution: It is essential to identify and protect the infraorbital nerve.

2. For direct visualization of the lateral maxillary wall as well as the fronto-zygomatic notch area, a retractor is placed in the fronto-zygomatic notch with lateral retraction exposing the areas highlighted (B).

- To assist in direct visualization of the drills during the preparation of the osteotomy, a "window" is made through the lateral maxillary wall as shown. Attempt to keep the Schneiderian membrane intact, if possible (B).

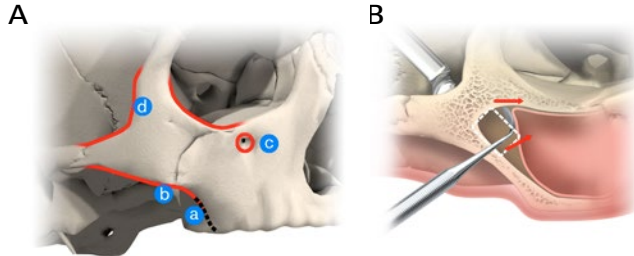


- Begin the trajectory of the implant at the first-second bicuspid area on the maxillary crest, follow the posterior maxillary wall and end at the lateral cortex of the zygomatic bone slightly inferior to the fronto-zygomatic notch (C).



- Drilling procedure: The ratio of the handpiece used is 20:1 at a speed of max. 2000rpm. Drill under constant and profuse irrigation by sterile saline at room temperature.

Caution: The Drill Guard may be used during the preparation of the osteotomy to avoid contact of the rotating drill with the adjacent soft tissues (D). Injury to the tongue, corner of the lips and or other soft tissues may occur if the drill shaft is unprotected.

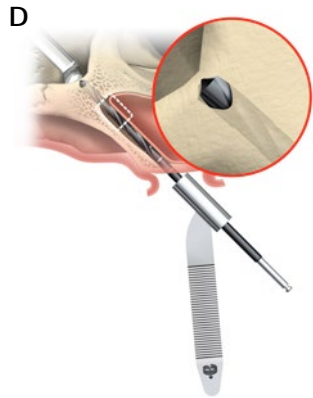

Depth measurement system: The parallel drills have a true depth measurement system. All drills and components are marked to prepare the site to the correct depth and obtain a secure and predictable position.

Caution: Pilot Drills extend up to 7.5mm longer than the implant when seated. Allow for this additional length when drilling near vital anatomical structures (please see image E for drill reference lines).

Caution: Avoid lateral pressure on drills during implant-site preparation. Lateral pressure may cause drill fracture.


Caution: Verify that drills lock in the handpiece before starting any drilling. A loose drill may accidentally harm the patient or members of the surgical team.

Caution: Verify that all interconnecting instruments lock properly before intraoral use to prevent accidental swallowing or aspiration.

- Drilling Sequence: (Image E shows relation between drills and implants). The initial osteotomy is made using the Brånemark System® Zygoma Round Bur, followed by the Brånemark System® Zygoma Twist Drill 2.9mm. Widening of the osteotomy is made by the Brånemark System® Zygoma Pilot Drill 3.5mm and finally the Brånemark System® Zygoma Twist Drill 3.5mm.

Caution: Ensure correct angulation and avoid drill wobble, as this can inadvertently widen the preparation site.

Caution: If the sinus membrane cannot be kept intact during osteotomy preparation, carefully irrigate away debris when inserting the implant. Any mucosal remnants in the bone site may prevent osseointegration of the implant.

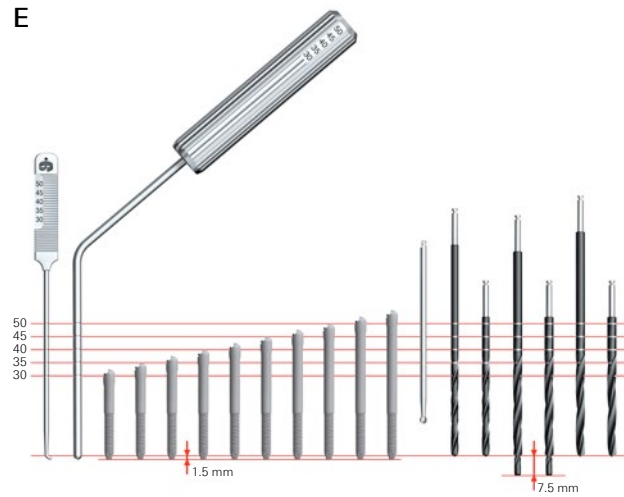

- Use the Z depth indicators to determine the length of the Zygoma implant to be placed. Copious irrigation of the sinus is recommended prior to implant placement.
- Plan to insert the implant as posteriorly as possible, with the implant head as close to the alveolar crest as possible (typically in the 2nd premolar region.) Anchorage of the implant will be achieved by entering the base of the zygoma bone (the posterior-lateral portion of the maxillary sinus roof), engaging through the lateral cortex of the zygoma below the frontozygomatic notch. Depending on the anatomy of the patient, the implant body may be positioned inside or outside the maxillary sinus.

Note: Adjustment to this implant placement may be considered due to anatomical variations in the maxilla as well as the maxillary sinus.

- Implant placement.

Insert implant with drilling unit:


The implant may be inserted using the drilling unit using **20 Ncm** insertion torque. Increasing the insertion torque up to maximum **50 Ncm** may be used for the complete seating of the implant (F). Once an insertion torque of **40 to 50 Ncm** is reached, the Z Handle may be used to tighten the implant manually to the proper insertion depth. Confirm through the "window" of the lateral maxillary wall the correct insertion angle of the implant while continuing through the sinus until the implant apex engages in the zygomatic bone.

Tighten manually:

Disengage the Connection to Handpiece from the implant mount and connect the Z Handle to the implant mount. Rotate the Z Handle clockwise until the desired depth and head position are achieved.

Caution: When using the Z Handle, applying excessive torque can distort the implant head or fracture the implant mount and/or the implant mount screw.

- Verifying the correct position of the implant platform: Place the Screwdriver Manual Unigrip™ into the implant mount screw (G). The shaft of the Unigrip™ driver should be perpendicular to the crest of the maxilla to ensure the proper position of the NobelZygoma™ 45° implant platform.

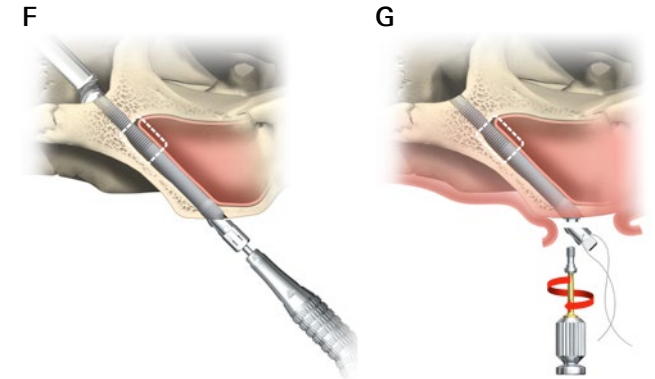

- Perform copious irrigation of the apical portion of the implant (the subperiosteal portion of the zygomatic bone) prior to the removal of the retractor from the fronto-zygomatic notch.
- Remove Implant mount.
- The premaxillary implants are placed following the conventional protocol for placement of implants.
- Depending on surgical protocol of choice, place a cover screw or abutment and suture. For Immediate Function, the implants should be able to withstand a final torque between **35–45 Ncm**. For two-stage protocol relieve the denture over the implants (H).

Caution: There are dedicated cover screws.



For additional information on surgical procedures please consult the Brånemark System® Zygoma "Procedures & products" treatment guidelines available at www.nobelbiocare.com or request latest printed version from a Nobel Biocare representative.

Materials:

NobelZygoma™ 45° implant: Commercially pure titanium grade 4.
 Cover Screw: Titanium alloy Ti-6Al-4V.
 Twist Drills and Pilot Drill: Stainless Steel with a DLC (Diamond Like Carbon) coating.
 Round Bur: Stainless Steel.
 Zygoma Handle: Aluminium alloy and stainless steel.
 Zygoma Drill Guard, Zygoma Drill Guard Short, Zygoma Depth Indicator Straight and Zygoma Depth Indicator Angled: Stainless steel.

Cleaning and sterilization:

NobelZygoma™ 45° implant and Cover Screw are delivered sterile and for single use only prior to the labeled expiration date.

Warning: Do not use device if the packaging has been damaged or previously opened.

Caution: NobelZygoma™ 45° implant, Twist Drills, Pilot Drill, Round Bur and Cover Screw are single use products and must not be reprocessed. Reprocessing could cause loss of mechanical, chemical and/or biological characteristics. Reuse could cause cross contamination.

Twist Drills, Pilot Drills and Round Burs are delivered non-sterile for single use. Prior to use clean, disinfect and sterilize the product using the recommended parameters.

Zygoma Handle, Zygoma Drill Guard, Zygoma Drill Guard Short, Zygoma Depth Indicator Straight and Zygoma Depth Indicator Angled are delivered non-sterile and are intended for re-use. Prior to use and re-use clean, disinfect and sterilize the products using the recommended parameters.

Warning: Use of non-sterile components may lead to infection of tissues or infectious diseases.

For USA: Seal single device in a pouch and steam sterilize at 270°F, max 279°F (132°C, max 137°C) for 3 minutes.

For outside USA: Seal single device in a pouch and steam sterilize at 132°C–135°C, max 137°C (270°F–275°F, max 279°F) for 3 minutes.

Alternative UK: Seal single device in a pouch and steam sterilize at 134°C–135°C, max 137°C (273°F–275°F, max 279°F) for 3 minutes.

Full set of recommended parameters are provided in “Cleaning & Sterilization Guidelines including MRI Information of Nobel Biocare Products” available at www.nobelbiocare.com/sterilization or request latest printed version from a Nobel Biocare representative.

Magnetic Resonance (MR) safety information:

Should there be no MR symbol on the product label, please note that this device has not been evaluated for safety and compatibility in the MR environment. This device has not been tested for heating or migration in the MR environment.

For additional information on Magnetic Resonance Imaging, please consult the “Cleaning & Sterilization Guidelines including MRI Information of Nobel Biocare Products” available at www.nobelbiocare.com or request latest printed version from a Nobel Biocare representative.

Storage and handling:

The product must be stored in a dry place in the original packaging at room temperature and not exposed to direct sunlight. Incorrect storage may influence device characteristics leading to failure.

Disposal:

Disposal of the device shall follow local regulations and environmental requirements, taking different contamination levels into account.

Manufacturer: Nobel Biocare AB, Box 5190, 402 26
 Västra Hamngatan 1, 411 17 Göteborg, Sweden.
 Phone: +46 31 81 88 00. Fax: +46 31 16 31 52. www.nobelbiocare.com



Canada license exemption: Please note that not all products may have been licensed in accordance with Canadian law.

Prescription device: Rx only

Caution: Federal law restricts this device to sale by or on the order of a licensed physician or dentist.

Symbols Glossary:

The following symbols may be present on the device labeling or in information accompanying the device. Refer to the device labeling or accompanying information for the applicable symbols.



Authorized representative in the European Community



Batch code



Catalogue number



Caution



CE marking



Consult instructions for use



Contains hazardous substances



Contains or presence of phthalate



Date



Date of manufacture



Do not resterilize



Do not re-use



Do not use if package is damaged



Double sterile barrier system

Rx Only

For prescription use only



Health care centre or doctor



Keep away from sunlight



Keep dry

symbol.glossary.nobelbiocare.com/ifu.nobelbiocare.com

Link to Online Symbols Glossary and IFU Portal



Magnetic resonance conditional



Manufacturer



Medical device



Non-pyrogenic



Non-sterile



Patient identification



Patient information website



Patient number



Serial number



Single sterile barrier system



Single sterile barrier system with protective packaging inside



Single sterile barrier system with protective packaging outside



Sterilized using ethylene oxide



Sterilized using irradiation



Temperature limit



Tooth number



Upper limit of temperature



Sterilized using steam or dry heat



Unique Device Identifier



Use-by date

EN All rights reserved.

Nobel Biocare, the Nobel Biocare logotype and all other trademarks used in this document are, if nothing else is stated or is evident from the context in a certain case, trademarks of Nobel Biocare. Product images in this folder are not necessarily to scale. All product images are for illustration purposes only and may not be an exact representation of the product.