

Bone Mill and Cover Screw Mill for Brånemark System®

Instructions for use



Important: Please read.

Disclaimer of liability:

This product is part of an overall concept and may only be used in conjunction with the associated original products according to the instructions and recommendation of Nobel Biocare. Non-recommended use of products made by third parties in conjunction with Nobel Biocare products will void any warranty or other obligation, express or implied, of Nobel Biocare. The user of Nobel Biocare products has the duty to determine whether or not any product is suitable for the particular patient and circumstances. Nobel Biocare disclaims any liability, express or implied, and shall have no responsibility for any direct, indirect, punitive or other damages, arising out of or in connection with any errors in professional judgment or practice in the use of Nobel Biocare products. The user is also obliged to study the latest developments in regard to this Nobel Biocare product and its applications regularly. In cases of doubt, the user has to contact Nobel Biocare. Since the utilization of this product is under the control of the user, they are his/her responsibility. Nobel Biocare does not assume any liability whatsoever for damage arising thereof. Please note that some products detailed in this Instruction for Use may not be regulatory cleared, released or licensed for sale in all markets.

Description:

The Bone Mills consist of a working part that cuts the outer periphery of the implant head free from bone and soft tissue. The working part also consists of a small guide peg, which centers the cutting part when placed in the inner canal of the implant.

The Cover Screw Mills consist of a working part that cuts the outer periphery of the cover screw free from bone and soft tissue. The working part also consists of a small guide peg that will centre the cutting part over the cover screw.

Both Bone Mill and Cover Screw Mill are compatible with Nobel Biocare external hex connection implants. Three different versions exist for NP, RP and WP external hex connections, all with corresponding laser marking.

Intended use:

The Bone Mills are used to remove any excessive bone around the implant platform to facilitate placement of prosthetic components.

The Cover Screw Mills are used to remove any bone or tissue overgrowth above the cover screw during a two-stage surgical procedure. This enables removal of the cover screw from the implant head.

Indications:

The Bone Mills are used to remove excess bone from around the coronal aspect of external hex connection implants NP, RP and WP.

The Cover Screw Mills are used for the removal of hard and soft tissue in conjunction with cover screws of external hex connection implants NP, RP and WP.

Contraindications:

In general, contraindications are applicable for implant surgery related procedures in patients:

- who are medically unfit for an oral surgical procedure.
- who are allergic or hypersensitive to medical grade stainless steel or any of its alloying components.

Warnings:

Besides the mandatory precautions for any surgery such as asepsis, during drilling in the jaw bone, one must avoid damage the nerves and vessels by referring to anatomical knowledge and preoperative radiographs.

Cautions:

It is strongly recommend that clinicians, new as well as experienced implant users, always go through special training before undertaking a new treatment method. Nobel Biocare offers a wide range of courses for various levels of knowledge and experience. For more information please visit www.nobelbiocare.com.

Working the first time with a colleague, experienced with a new device/treatment method, will provide further insight and understanding. Nobel Biocare has a global network of mentors available for this purpose.

All instruments and tooling used in surgery must be maintained in good condition and care must be taken that instrumentation does not damage implants or other components.

Because of the small size of the devices, care must be taken that they are not swallowed or aspirated by the patient.


Only use each Bone Mill and Cover Screw Mill with the respective implant dimension mentioned above, as damage to the implant head and inner threads could occur otherwise.

Handling procedure:

Both the Bone Mill and Cover Screw Mill are used during the second-stage surgery as part of the two-stage surgical procedure. The Bone Mill can also be used during single-stage surgery before placing the abutment. Both instruments are designed to be used by hand.

Procedure:

1. Uncover the implant by making an incision to expose cover screw or use the Soft Tissue Punch in case of sufficient amount of attached mucosa.
2. Place the guide peg of the Cover Screw Mill in the central hole of the cover screw head. Bone or connective tissue is removed by gently rotating the instrument.
3. Remove cover screw using Cover Screw Driver Brånemark System® Hexagon.
4. Place the guide peg of the Bone Mill in the inner canal of the implant. Press the Bone Mill slightly towards the implant head and gently rotate the instrument to remove any bone around the implant platform that may hinder an abutment from being fully seated on the implant. Please note that the Bone Mill can also be used independently during surgery without cover screw milling.

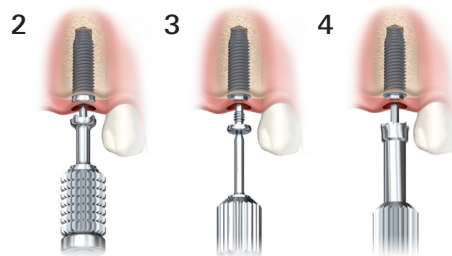

5. When the surrounding bone and tissue close to the implant platform has been sufficiently reduced, it is ready for abutment connection. Ensure that the implant platform is clean from bone remnants.

For additional information on surgical procedures please consult the procedures manual for the respective implant system available at www.nobelbiocare.com or request latest printed version from a Nobel Biocare representative.

Materials:

Bone Mill and Cover Screw Mill: medical grade stainless steel.

Cleaning and sterilization instructions:

The device is delivered non-sterile and intended for re-use. This device must be cleaned and sterilized prior to use

For USA: Seal single device in a pouch and steam sterilize at 270°F (132°C) for 3 minutes.

For outside USA: Seal single device in a pouch and steam sterilize at 132°C–135°C (270°F–275°F) for 3 minutes.

Alternative UK: Seal single device in a pouch and steam sterilize at 134°C–135°C (273°F–275°F) for 3 minutes.

Full set of recommended parameters are provided in "Cleaning & sterilization guidelines for Nobel Biocare products including MRI information" available at www.nobelbiocare.com/sterilization or request latest printed version from a Nobel Biocare representative.

Warning: Use of non-sterile components may lead to infection of tissues or infectious diseases.

MRI safety information:


Please note that the product has not been evaluated for safety and compatibility in the MR environment. The product has not been tested for heating or migration in the MR environment.

Storage and handling:

The product must be stored in a dry place in the original packaging at room temperature and not exposed to direct sunlight. Incorrect storage may influence device characteristics leading to failure.

Disposal:

Disposal of the device shall follow local regulations and environmental requirements, taking different contamination levels into account.

 **Manufacturer:** Nobel Biocare AB, Box 5190, 402 26 Västra Hamngatan 1, 411 17 Göteborg, Sweden.
Phone: +46 31 81 88 00. Fax: +46 31 16 31 52. www.nobelbiocare.com



Canada license exemption: Please note that not all products may have been licensed in accordance with Canadian law.

Prescription device: Rx only

Caution: Federal law restricts this device to sale by or on the order of a licensed physician or dentist.

Symbols Glossary:

The following symbols may be present on the device labeling or in information accompanying the device. Refer to the device labeling or accompanying information for the applicable symbols.



Authorized representative in the European Community



Batch code



Catalogue number



Caution



CE marking



Consult instructions for use



Contains hazardous substances



Contains or presence of phthalate



Date



Date of manufacture



Do not resterilize



Do not re-use



Do not use if package is damaged



Double sterile barrier system

Rx Only

For prescription use only



Health care centre or doctor



Keep away from sunlight



Keep dry



symbol.glossary.nobelbiocare.com
ifu.nobelbiocare.com

Link to Online Symbols Glossary and IFU Portal



Magnetic resonance conditional



Manufacturer



Medical device



Non-pyrogenic



Non-sterile



Patient identification



Patient information website



Patient number



Serial number



Single sterile barrier system



Single sterile barrier system with protective packaging inside



Single sterile barrier system with protective packaging outside



Sterilized using ethylene oxide



Sterilized using irradiation



Temperature limit



Tooth number



Upper limit of temperature



Sterilized using steam or dry heat



Unique Device Identifier



Use-by date

EN All rights reserved.

Nobel Biocare, the Nobel Biocare logotype and all other trademarks used in this document are, if nothing else is stated or is evident from the context in a certain case, trademarks of Nobel Biocare. Product images in this folder are not necessarily to scale. All product images are for illustration purposes only and may not be an exact representation of the product.